



A commentary by J. Chris Coetzee, MD, FAAOS, is linked to the online version of this article.

Three-Year Rates of Reoperation and Revision Following Mobile Versus Fixed-Bearing Total Ankle Arthroplasty

A Cohort of 302 Patients with 2 Implants of Similar Design

M. Assal, MD, H. Kutaish, MD, A. Acker, MD, J. Hattendorf, PhD, A. Lübbecke, MD, DSc, and X. Crevoisier, MD

Investigation performed at Geneva University Hospitals, Geneva; Lausanne University Hospitals (CHUV), Lausanne; and the Centre of Foot and Ankle Surgery, Clinique La Colline, Geneva, Switzerland

Background: Currently, the implants utilized in total ankle arthroplasty (TAA) are divided between mobile-bearing 3-component and fixed-bearing 2-component designs. The literature evaluating the influence of this mobility difference on implant survival is sparse. The purpose of the present study was therefore to compare the short-term survival of 2 implants of similar design from the same manufacturer, surgically implanted by the same surgeons, in fixed-bearing or mobile-bearing versions.

Methods: All patients were enrolled who underwent TAA with either the mobile-bearing Salto (Tornier and Integra) or the fixed-bearing Salto Talaris (Integra) in 3 centers by 2 surgeons between January 2004 and March 2018. All patients who underwent TAA from January 2004 to April 2013 received the Salto implant, and all patients who underwent TAA after November 2012 received the Salto Talaris implant. The primary outcome was time, within 3 years, to first all-cause reoperation, revision of any metal component, and revision of any component, including the polyethylene insert. Secondary outcomes included the frequency, cause, and type of reoperation.

Results: A total of 302 consecutive patients were included, of whom 171 received the mobile-bearing and 131 received the fixed-bearing implant. The adjusted hazard ratio for all-cause reoperation was 1.42 (95% confidence interval [CI], 0.67 to 3.00; $p = 0.36$); for component revision, 3.31 (95% CI, 0.93 to 11.79; $p = 0.06$); and for metal component revision, 2.78 (95% CI, 0.58 to 13.33; $p = 0.20$). A total of 31 reoperations were performed in the mobile-bearing group compared with 14 in the fixed-bearing group ($p = 0.07$). More extensive reoperation procedures were performed in the mobile-bearing group.

Conclusions: With the largest comparison of 2 implants of similar design from the same manufacturer, the present study supports the use of a fixed-bearing design in terms of short-term failure. We found a 3-times higher rate of revision among mobile-bearing implants compared with fixed-bearing implants at 3 years after TAA. Reoperations, including first and subsequent procedures, tended to be less common and the causes and types of reoperations less extensive among fixed-bearing implants.

Level of Evidence: Therapeutic Level III. See Instructions for Authors for a complete description of levels of evidence.

Total ankle arthroplasty (TAA) is increasingly utilized to treat end-stage osteoarthritis because of the biomechanical advantages of arthroplasty over arthrodesis^{1,2}

and the promising mid-term and long-term outcomes³⁻⁵. Despite its success, TAA is historically associated with higher rates of early reoperation and revision compared with total

Disclosure: The **Disclosure of Potential Conflicts of Interest** forms are provided with the online version of the article (<http://links.lww.com/JBJS/G666>).

Copyright © 2021 The Authors. Published by The Journal of Bone and Joint Surgery, Incorporated. All rights reserved. This is an open-access article distributed under the terms of the [Creative Commons Attribution-Non Commercial-No Derivatives License 4.0](https://creativecommons.org/licenses/by-nc-nd/4.0/) (CCBY-NC-ND), where it is permissible to download and share the work provided it is properly cited. The work cannot be changed in any way or used commercially without permission from the journal.







Fig. 1-A

Fig. 1-B

Figs. 1-A and 1-B Images of the Salto mobile-bearing (**Fig. 1-A**) and Salto Talaris fixed-bearing (**Fig. 1-B**) implants.

hip and knee arthroplasty⁶⁻⁹, which demonstrates the difficulty of replacing the relatively complex ankle joint^{9,10}.

Nevertheless, continuous advances in implant design have improved outcomes and survival rates of TAA^{11,12}. Current implants are divided between mobile-bearing 3-component and fixed-bearing 2-component designs. Most comparative clinical studies and meta-analyses have not demonstrated differences in reoperation and revision rates between implant designs¹³⁻¹⁶. However, the latest registry reports and a systematic review have demonstrated a new trend toward the superiority of fixed-bearing 2-component designs in terms of the rates of reoperation and revision¹⁷⁻¹⁹.

Mobile-bearing implants have exhibited increased rates of instability and subluxation of the polyethylene component²⁰, whereas fixed-bearing implants have been associated with a higher rate of tibial loosening and polyethylene wear, likely as a result of shear forces^{16,21}. However, a finite-element analysis found no dif-

ferences in bone strain or bone-implant interfacial stress between 2 comparable fixed-bearing and mobile-bearing implants²². Fixed-bearing designs have benefited from a series of design improvements over the years, and a recent study reported no major strain differences between mobile-bearing and fixed-bearing designs²². Furthermore, newer designs have corrected many of the flaws of previous generations, casting doubt on the relevance of these older observations in the context of modern TAA implants²³. Therefore, early identification of complications related to implant design remains a major challenge in the field of ankle arthroplasty^{11,24}.

The purpose of the present study was therefore to compare the short-term survival of 2 implants of similar design from the same manufacturer, surgically implanted by the same surgeons, in fixed-bearing or mobile-bearing versions, and to evaluate the frequency, cause, and type of procedures associated with reoperations.

Materials and Methods

Patients and Study Design

All patients were enrolled who underwent TAA with either the mobile-bearing Salto (Tornier and Integra) or the fixed-bearing Salto Talaris (Integra) at 3 centers (Geneva University Hospitals; Clinique La Colline Hirslanden, Centre of Foot and Ankle Surgery in Geneva; and Lausanne University Hospital) between January 2004 and March 2018. Two surgeons (M.A. and X.C.) performed all of the TAA procedures together. All patients who underwent TAA from January 2004 to November 2012 received the mobile-bearing Salto implant, and all patients who underwent TAA after April 2013 received the fixed-bearing Salto Talaris implant, with patients treated in the short intervening period receiving one of these implants according to availability. No deaths occurred within the first 3 years postoperatively, and no patients were excluded from the study. The study was approved by the relevant national ethics boards (Swiss Ethics, project ID 2016-00065).

Demographics and Outcomes

Demographic variables were noted at the time of patient inclusion, with the exception of the body mass index and American Society of Anesthesiologists (ASA) score, which were collected retrospectively from patient files so as to assess the possible heterogeneity of the baseline characteristics.

The primary outcome was the time to first all-cause reoperation, defined as any procedure on the ankle and/or any of the adjacent joints following the index procedure. The 2 end points relating to revision reflect 2 common definitions of revision in the literature: (1) revision for the exchange of metal components or for conversion to salvage arthrodesis^{25,26} and (2) revision of any component, including isolated polyethylene exchange, or for conversion to salvage arthrodesis¹⁸.

Secondary outcomes were the frequency (number of first and subsequent reoperations), cause, and type of reoperation, graded in accordance with other published work^{26,27}. All patients had standard radiographs at 3 months and 1 year postoperatively, and then every other year thereafter. In addition, patients with painful prostheses were further assessed with use of computed tomography. Patient symptoms and imaging results were assessed to determine the necessity of a reoperation.

Implants

The mobile-bearing Salto implant was introduced to the European market in 1997, and the fixed-bearing Salto Talaris implant was introduced in 2012 (Figs. 1-A and 1-B). The tibial and talar components of both prostheses are made of cobalt-chromium alloy. The coating of the Salto mobile-bearing prosthesis consists of plasma spray titanium and hydroxyapatite. Hydroxyapatite was not utilized in the coating of the Salto Talaris. Both prostheses are of anatomical design and are implanted cementless with a standard bone resection of 7 mm. In both prostheses, the talar component is conical in shape with 2 different radii of curvature to match the normal morphology of the talus. Fixation of the talar component is press-fit and enhanced by a central peg.

The tibial part utilizes a central press-fit keel for fixation. In the fixed-bearing design, the polyethylene is fixed to the tibial component, whereas in the mobile-bearing design, the polyethylene is positioned between the tibial and talar components, thus creating 2 articulating surfaces. Regarding the learning curve for implantation, both surgeons had extensive experience utilizing the Salto implant during TAA since the year 2000. Further, because the surgical technique and the instrumentation of both models are identical, there was no learning curve adapting to the new fixed-bearing model.

Surgical Technique and Rehabilitation

The prosthesis was implanted through an anterior approach between the tibialis anterior and extensor hallucis longus tendons. A pneumatic thigh tourniquet was utilized in all cases, being inflated immediately prior to the skin incision and kept until closure. Attention was paid to create a plantigrade foot and a balanced ankle, as achieved with use of selected adjunctive procedures. Patients were allowed to walk with partial weight-bearing (20 kg) on postoperative day 3. A protective cast was utilized for 6 weeks postoperatively, after which passive and active range of motion were begun.

Statistical Analyses

Data were summarized with use of descriptive statistics. For the primary outcome, Kaplan-Meier survival analysis was performed for 3 different end points: (1) all-cause reoperation, (2) revision for the exchange of metal components or for conversion to salvage arthrodesis, and (3) revision of any component, including isolated polyethylene exchange, or for conversion to

TABLE I Patient Demographics*

	Mobile-Bearing (N = 171)	Fixed-Bearing (N = 131)
Age (yr)	62 ± 12	68 ± 9
Body mass index (kg/m ²)	28.0 ± 7.0	27.6 ± 5.1
Male sex male	87 (51%)	63 (48%)
Indication, posttraumatic arthritis	139 (81%)	109 (83%)
Diabetes	5 (3%)	7 (5%)
ASA score		
1 or 2	107 (87%)	95 (85%)
3 or 4	16 (13%)	17 (15%)
Hindfoot alignment		
Neutral	133 (78%)	71 (54%)
Varus	14 (8%)	24 (18%)
Valgus	24 (14%)	36 (28%)

*Values are given as the mean ± standard deviation or as the count with the percentage in parentheses. Body mass index had missing data for 55 patients in the mobile-bearing group and 16 in the fixed-bearing group. ASA score had missing data for 48 patients in the mobile-bearing group and 12 in the fixed-bearing group.

TABLE II Unadjusted and Adjusted HRs for Reoperation and Revision

	Patient N (%)	Survival					
		Unadjusted HR (95% CI)	P Value	Adjusted HR* (95% CI)	P Value	Adjusted HR† (95% CI)	P Value
Reoperation							
Mobile-bearing	22 (12.9%)						
Fixed-bearing	11 (8.4%)	1.57 (0.76-3.24)	0.22	1.42 (0.67-3.00)	0.36	NA‡	
Revision (polyethylene exchange included)							
Mobile-bearing	14 (8.2%)						
Fixed-bearing	3 (2.3%)	3.70 (1.06-12.86)	0.04	3.31 (0.93-11.79)	0.06	3.70§ (1.06-12.86)	0.04
Revision (polyethylene exchange excluded)							
Mobile-bearing	8 (4.7%)						
Fixed-bearing	2 (1.5%)	3.14 (0.66-14.82)	0.12	2.78 (0.58-13.33)	0.20	2.79# (0.59-13.12)	0.20

*Analysis adjusted for covariates with substantial baseline imbalance (i.e., age and alignment). †According to best-fit model (determined by smallest Akaike information criterion). ‡The null model was the model with the lowest Akaike information criterion (373.2). NA = not available. §The unadjusted model was the model with the lowest Akaike information criterion (189.8). #The model adjusted for alignment showed best fit (Akaike information criterion: 113.1).

salvage arthrodesis. Charts were audited for any patient who did not undergo a reoperation in order to confirm that no reoperation had occurred within 3 years postoperatively. Corresponding p values were calculated with use of the log-rank test. To compare the 3-year outcomes of the 2 types of implants, unadjusted hazard ratios (HRs) and 95% confidence intervals (CIs) were estimated with use of Cox regression analysis. To account for baseline imbalances in age⁹ and alignment²⁸, an additional Cox regression analysis was performed adjusting for these variables. In addition, we identified the best regression model by testing all possible combinations of the predictor variables age, sex, alignment, and posttraumatic or other indication. The model with the lowest Akaike information criterion was considered to be the best-fit model. Finally, the incidence of reoperation was calculated with use of Poisson regression analysis, with reoperation per person-year as the outcome. All analyses were performed independently by a senior statistician (A.L.) and an epidemiologist statistician (J.H.) with use of R (version 3.5.0; R Foundation for Statistical Computing), SPSS (version 25; IBM), and Stata (version 15; StataCorp).

Source of Funding

We received internal funding from our institutions and external funding in the form of a research grant from the Swiss Foot and Ankle Society, which did not play a role in the investigation.

Results

Overall, a total of 302 consecutive patients were included, of whom 171 received a mobile-bearing implant and 131 received a fixed-bearing implant. Patient demographics were comparable between groups in terms of patient sex, body mass index, diabetes, and ASA score distribution. A greater proportion of patients had valgus-aligned ankles in the fixed-bearing group, and the fixed-bearing group had a higher mean

age (Table I). No patient was lost to follow-up at the time of the 3-year evaluation.

Regarding the primary outcome, 22 patients (12.9%) in the mobile-bearing group underwent ≥ 1 reoperation compared with 11 (8.4%) in the fixed-bearing group (Table II). The 3-year rate of survival free from any reoperation was 87.1% (95% CI, 82.3% to 92.3%) in the mobile-bearing group compared with 91.6% (95% CI, 87.0% to 96.5%) in the fixed-bearing group (log-rank test, $p = 0.21$) (Fig. 2). The adjusted HR for any reoperation was 1.42 (95% CI, 0.67 to 3.00; $p = 0.36$) (Table II). The most common reoperation procedures were cyst debridement, gutter debridement (i.e., the removal of impinging bone at the medial or lateral side of the implant), salvage arthrodesis, wound debridement, and polyethylene




Fig. 2
Three-year Kaplan-Meier survival analysis of the mobile-bearing and fixed-bearing groups, with any reoperation as end point.

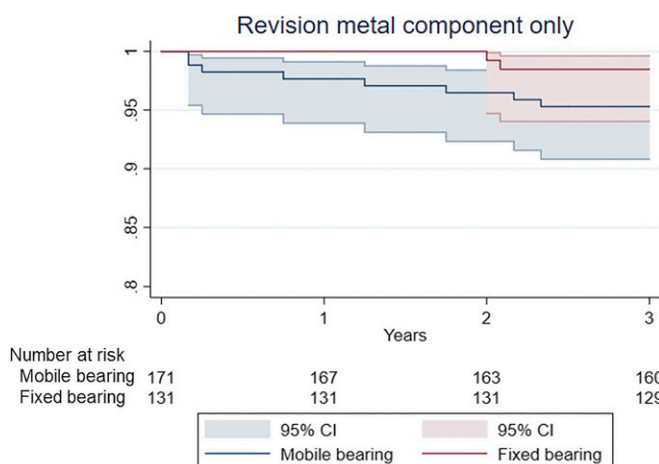


Fig. 3-A

Fig. 3-A Three-year Kaplan-Meier survival analysis of the mobile-bearing and fixed-bearing groups, with revision of any metal components as the end point.

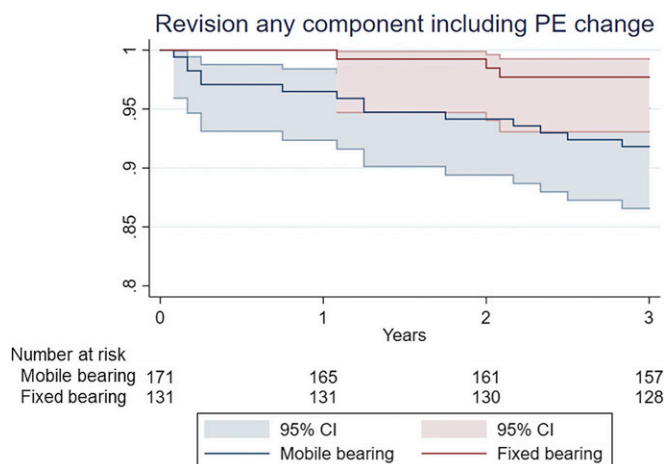


Fig. 3-B

Fig. 3-B Three-year Kaplan-Meier survival analysis of the mobile-bearing and fixed-bearing groups, with revision of any component, including isolated polyethylene (PE) exchange, as the end point.

exchange in the mobile-bearing group and gutter debridement, wound debridement, salvage arthrodesis, and ligamentoplasty in the fixed-bearing group.

Fourteen patients (8.2%) in the mobile-bearing group underwent revision of any component, including polyethylene exchange, compared with 3 (2.3%) in the fixed-bearing group (Table II). The 3-year rate of survival for revision of any component was 91.8% (95% CI, 87.8% to 96.0%) in the mobile-bearing group compared with 97.7% (95% CI, 95.2% to 99.9%) in the fixed-bearing group (log-rank test, $p = 0.03$) (Fig. 3-A), and the adjusted HR was 3.31 (95% CI, 0.93 to 11.79; $p = 0.06$). At the time of the latest follow-up, an additional 2 patients in the mobile-bearing group had planned revision for polyethylene exchange compared with none in the fixed-bearing group.

Eight patients (4.7%) in the mobile-bearing group underwent revision of a metal component compared with 2 (1.5%) in the fixed-bearing group. The 3-year rate of survival for revision of any metal component was 95.3% (95% CI, 92.2% to 98.5%) in the mobile-bearing group compared with 98.5% (95% CI, 96.4% to >99.9%) in the fixed-bearing group (log-rank test $p = 0.13$) (Fig. 3-B). The adjusted HR for revision of any metal component was 2.78 (95% CI, 0.58 to 13.33; $p = 0.20$). When visualizing the Kaplan-Meier survival analysis (Figs. 3-A and 3-B), the immediate drops in survival could be attributed to 5 patients: 2 with an early deep infection, 2 with polyethylene subluxation, and 1 with an atraumatic medial malleolar fracture.

Regarding the secondary outcomes, 33 (10.9%) of the 302 patients in the study group underwent ≥ 1 reoperation (10.9%), of whom 12 (4.0%) underwent ≥ 2 reoperations. A total of 31 reoperations, including both first and subsequent reoperations, were performed in 22 patients (12.9%) in the mobile-bearing group compared with 14 reoperations in 11 (8.4%) in the fixed-bearing group (HR, 1.70; 95% CI, 0.94 to 3.06; $p = 0.07$) (Table III). A total of 54 procedures were

performed during those 31 reoperations in the mobile-bearing group compared with 16 procedures during 14 reoperations in the fixed-bearing group. The mobile-bearing

TABLE III Causes and Types of Reoperation Procedures Performed

	Mobile-Bearing Group (N = 171)	Fixed-Bearing Group (N = 131)
No. of patients	22	11
No. of reoperations	31	14
Cause for reoperation*		
Wound-healing problem	7 (4.1%)	4 (3.0%)
Infection	3 (1.7%)	2 (1.5%)
Gutter impingement	8 (4.7%)	5 (3.8%)
Fracture	1 (0.6%)	0 (0.0%)
Polyethylene subluxation	2 (1.2%)	0 (0.0%)
Polyethylene wear	5 (2.9%)	1 (0.8%)
Cyst	9 (5.3%)	1 (0.8%)
Loosening	2 (1.2%)	1 (0.8%)
Adjacent joint arthrosis	5 (2.9%)	0 (0.0%)
Reoperation procedure*		
Wound debridement	7 (4.1%)	4 (3.1%)
Osteosynthesis	1 (0.6%)	0 (0.0%)
Polyethylene exchange	7 (4.1%)	1 (0.8%)
Gutter debridement	8 (4.7%)	5 (3.8%)
Cyst debridement	11 (6.4%)	1 (0.8%)
Adjacent joint fusion	5 (2.9%)	0 (0.0%)
Ligamentoplasty	2 (1.2%)	2 (1.5%)
Metal component exchange	6 (3.5%)	1 (0.8%)
Salvage arthrodesis	7 (4.1%)	2 (1.5%)

*Some reoperations were performed for multiple causes and included multiple procedures.

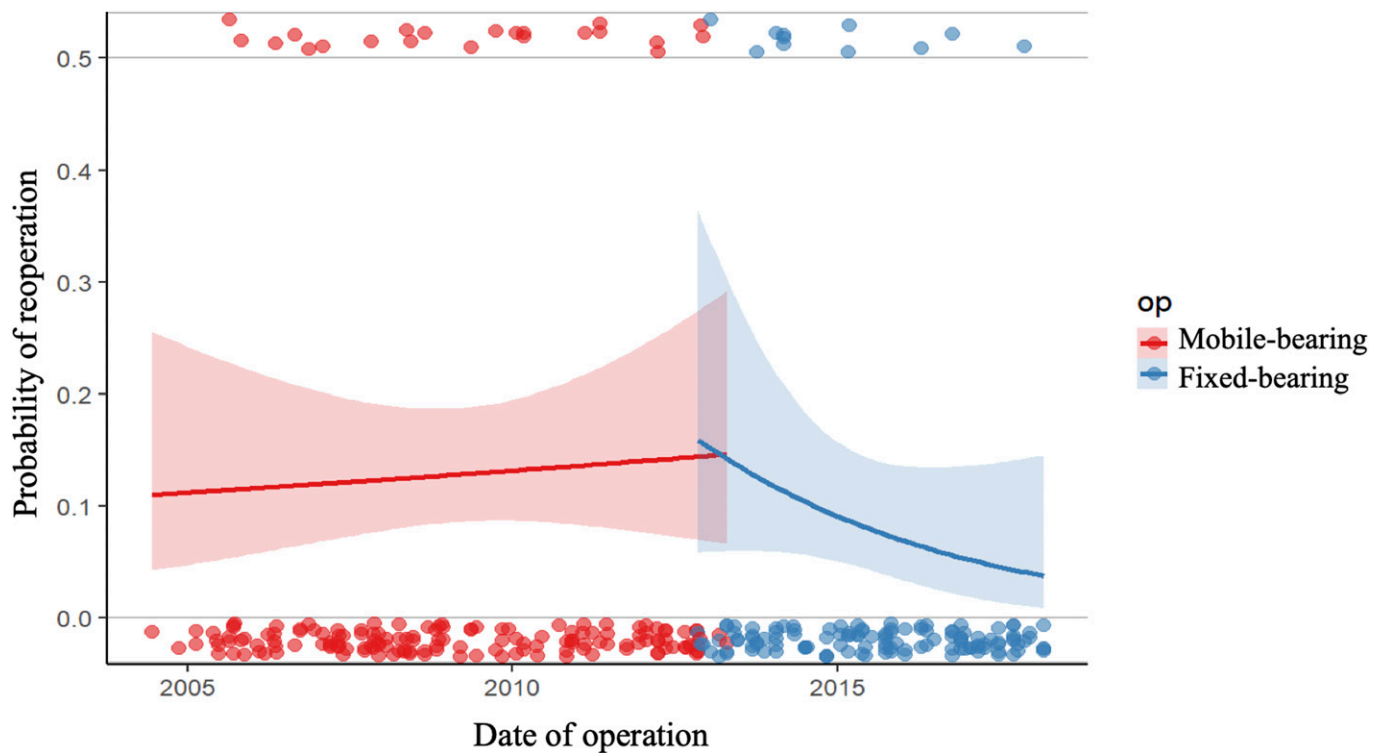


Fig. 4

Probability of reoperation over time for the mobile-bearing and fixed-bearing groups, calculated with use of a Poisson regression model, with reoperations per person-year as the outcome.

group underwent proportionally more polyethylene exchange (4.1%) and cyst debridement (6.4%) than the fixed-bearing group (0.8% for both procedures). Finally, although the probability of reoperation marginally increased over time in the mobile-bearing group, it decreased in the fixed-bearing group (Fig. 4).

Discussion

The purpose of the present study was to compare the short-term survival of 2 implants of similar design from the same manufacturer, surgically implanted by the same surgeons, in fixed-bearing or mobile-bearing versions. We observed an approximately 3-times greater rate of all-cause revision in the mobile-bearing group compared with the fixed-bearing group at 3 years after TAA. There were fewer reoperations, including first and subsequent reoperations, in the fixed-bearing group, with reoperations involving fewer procedures performed for less severe complications.

To our knowledge, the present study is the first comparative clinical study to evaluate the influence of bearing type on implant survival in prostheses of similar design from the same manufacturer. Previous case series have shown a large variability in the rates of revision and reoperation associated with these implants (Table IV). The present results are consistent with the those reported in the 2019 annual report of the Australian Orthopaedic Association National Joint Replacement Registry (AOANJRR)¹⁸, which indicated a

3-year cumulative percent revision of 1.8% (95% CI, 0.7% to 4.3%) for the Salto Talaris fixed-bearing implant (n = 344) compared with 6.1% (95% CI, 4.1% to 9.0%) for the Salto mobile-bearing implant (n = 415). The registry showed that the Salto Talaris had the best 3-year survival among all of the included implants. The overall 3-year cumulative incidence of revision was 2.2% (95% CI, 1.1% to 4.5%) for all of the included fixed-bearing implants and 7.3% (95% CI, 6.4% to 12.8%) for all of the included mobile-bearing implants. Moreover, the New Zealand Registry reported no revisions in 98 TAAs performed with the Salto Talaris (rate per 100 component years, 0) compared with 53 revisions in 721 TAAs performed with the Salto (rate per 100 component years, 1.34)¹⁷.

In the present study, the most common reoperation procedures were cyst debridement, gutter debridement (i.e., the removal of impinging bone at the medial or lateral side of the implant), salvage arthrodesis, wound debridement, and polyethylene exchange in the mobile-bearing group and gutter debridement, wound debridement, salvage arthrodesis, and ligamentoplasty in the fixed-bearing group. The greater proportion of isolated polyethylene exchange observed in the mobile-bearing group was in accordance with the 2019 annual report of the AOANJRR¹⁸, which identified isolated polyethylene exchange as the cause of >50% of the revisions associated with these prostheses. We also observed that the mobile-bearing group underwent a greater number of reoperations for cyst de

TABLE IV Literature Review of the Reported Reoperation and Revision Rates of the Salto and Salto Talaris Implants*

	Study	Journal	No. of Procedures	Minimum Follow-up (mo)	Reoperation Rate (%)	Revision Rate (Polyethylene Exchange Included)	Revision Rate (Polyethylene Exchange Excluded)
Salto	Present study	-	171	36	12.9%	8.2%	4.7%
	Mehdi ³⁴ , 2019	OTSR	25	40	25.0%	10.0%	10.0%
	Koo ³⁵ , 2019	FAI	55	24	9.8%	6.7%	6.7%
	Wan ¹⁰ , 2018	FAI	59	6	11.9%	5.1%	5.1%
	Gaudot ¹³ , 2014	FAI	33	4	12.1%	0.0%	0.0%
	Rodrigues-Pinto ³⁶ , 2013	FAS	119	18	5.9%	2.7%	2.7%
	Schenk ³⁷ , 2011	FAI	218	24	11.0%	-	5.5%
	Reuver ³⁸ , 2010	FAI	59	12	16.9%	-	11.9%
	Bonnin ³⁹ , 2011	CORR	98	81.6	35.0%	20.1%	15.0%
	Bonnin ⁴⁰ , 2004	CORR	93	24	4.3%	2.2%	2.2%
Salto Talaris	Present study	-	131	30	8.4%	2.3%	1.5%
	Nunley ¹⁴ , 2019	FAI	43	24	7.0%	7.0%	2.3%
	Marks ⁴¹ , 2019	JFAS	50	11	12.0%	2.0%	0.0%
	Cody ⁴² , 2019	FAI	79	60	-	8.8%	8.8%
	Pangrazzi ⁴³ , 2018	FAI	104	20	11.0%	5.0%	5.0%
	Stewart ⁴⁴ , 2017	FAI	72	60	19.0%	5.1%	3.8%
	Hofmann ⁴⁵ , 2016	JBJS	81	41	21.0%	-	2.5%
	Oliver ⁴⁶ , 2016	FAI	321	24	6.2%	-	2.8%
	Chao ⁴⁷ , 2015	FAI	23	24	17.4%	-	4.6%
	Nodzo ⁴⁸ , 2014	FAI	75	24	17.3%	-	2.0%
	Gaudot ¹³ , 2014	FAI	33	11	3.0%	3.0%	3.0%
	Schweitzer ⁴⁹ , 2013	JBJS	67	24	12.0%	3.0%	3.0%
	Both (mixed)	Gramlich ⁵⁰ , 2018	IO	60	24	42.0%	15.0%

*OTSR = Orthopaedics & Traumatology: Surgery and Research, FAI = Foot and Ankle International, JFAS = Journal of Foot & Ankle Surgery, CORR = Clinical Orthopaedics and Related Research, JBJS = Journal of Bone and Joint Surgery, IO = International Orthopaedics, and FAS = Foot and Ankle Surgery.

bridement over 3 years compared with the fixed-bearing group; this observation is in accordance with previous reports comparing mobile- and fixed-bearing implants^{13,14}. In our practice, the presence of a symptomatic cyst is confirmed with use of computed tomography²⁹. The cysts are then treated surgically by debridement and grafting, usually in combination with adjunctive surgical procedures, which may include component exchange. Although the reason for the formation of such cysts following TAA remains unclear, it is likely multifactorial, including an interaction with the particles resulting from polyethylene wear, micromotions, and hydroxyapatite coating^{30,32}. Previous studies have shown that polyethylene particles are not the primary cause of osteolytic cyst formation but are a secondary factor that might contribute to the acceleration of osteolysis^{30,33}. The 2019 report from the AOANJRR¹⁸ indicated that there was presently no evidence that the coating of an implant affects the rate of revision following TAA.

In the present study, patients who received a mobile-bearing implant were more likely to undergo reoperations for a

more severe complication than those who received a fixed-bearing implant, including higher rates of metal component exchange and salvage arthrodesis. The 3 most common reasons for reoperation were symptomatic cysts, gutter impingement, and wound-healing complications in the mobile-bearing group and gutter impingement, wound-healing complications, and deep infection in the fixed-bearing group.

When visualizing the Kaplan-Meier survival analysis (Figs. 3-A and 3-B), the immediate drops in survival could be attributed to 5 patients: 2 with an early deep infection, 2 with polyethylene luxation (which is a complication that is specific to the mobile-bearing design), and 1 with an atraumatic medial malleolar fracture. The rate of infection was similar between groups (1.7% in the mobile-bearing group and 1.5% in the fixed-bearing group), but infections occurred earlier in the mobile-bearing group.

One strength of the present study was that it represented the largest direct comparison of 2 implants of similar design from the same manufacturer, surgically implanted by the same

surgeons, in fixed-bearing or mobile-bearing versions, which allowed us to analyze the effect of design on short-term implant survival. However, 1 limitation of the study was that the study design did not allow for randomization because the fixed-bearing implant was not being manufactured at the beginning of the recruitment process. Although we could not exclude the possibility of a learning effect, we believe that any such effect would be small because the 2 operating surgeons had substantial experience in TAA prior to the commencement of the study, specifically with the Salto implant as they started using this prosthesis in 2000 and the study period began in 2004. Additionally, in the mobile-bearing group, 10 of 86 patients in the first chronological half of the study underwent ≥ 1 reoperation compared with 12 of 85 patients in the second chronological half. Figure 4 shows that the probability of reoperation in the mobile-bearing group was consistent over the duration that this implant was utilized.

After adjusting for the baseline differences in age and alignment, the HR slightly changed and the CI included 1, indicating a loss of statistical significance. However, 2 patients in the mobile-bearing group had planned revision for polyethylene exchange compared with none in the fixed-bearing group. Overall, the number of events was relatively small, affecting the precision of our analyses. The analysis may also have been slightly affected by the younger age and greater proportion of valgus-aligned ankles in the fixed-bearing group. An effect of these parameters on the risk has been described in the literature^{9,28}, although other studies have suggested that alignment does not substantially affect the rate of failure in TAA^{11,28}. Nonetheless, neither adjustment for age and alignment nor for other sets of covariates had a noteworthy effect on point or interval survival estimates. Finally, the decision to perform a reoperation following TAA is complex and likely surgeon-dependent; however, the same 2 surgeons performed all of the index procedures and reoperations throughout the study period.

Conclusions

On the basis of the largest comparison of survival between 2 implants of similar design from the same manufacturer, the present study supports the use of a fixed-bearing implant in TAA. We found a 3-times higher rate of revision for TAAs performed with the Salto mobile-bearing implant compared with the Salto Talaris fixed-bearing implant at 3 years after TAA. There were fewer reoperations, including first and subsequent reoperations, in the fixed-bearing group, with reoperations involving fewer procedures performed for less severe complications. ■

Note: The authors thank Richard Stern, MD, and Jeremy Valluy, PhD, for their contributions to the scientific writing and editing of this manuscript.

M. Assal, MD^{1,2}
H. Kutaish, MD^{1,2}
A. Acker, MD¹
J. Hattendorf, PhD^{3,4}
A. Lübbeke, MD, DSc^{2,5}
X. Crevoisier, MD⁶

¹Centre of Foot and Ankle Surgery, Clinique La Colline, Geneva, Switzerland

²Faculty of Medicine, University of Geneva, Geneva, Switzerland

³Department of Epidemiology and Public Health, Swiss Tropical and Public Health Institute, Basel, Switzerland

⁴Basel University, Basel, Switzerland

⁵Geneva University Hospitals, Geneva, Switzerland

⁶Lausanne University Hospitals (CHUV) and University of Lausanne (UNIL), Lausanne, Switzerland

Email for corresponding author: hala.kutaish@gmail.com

References

- Chopra S, Rouhani H, Assal M, Aminian K, Crevoisier X. Outcome of unilateral ankle arthrodesis and total ankle replacement in terms of bilateral gait mechanics. *J Orthop Res*. 2014 Mar;32(3):377-84.
- Valderrabano V, Nigg BM, von Tscharnner V, Frank CB, Hintermann B. J. Leonard Goldner Award 2006. Total ankle replacement in ankle osteoarthritis: an analysis of muscle rehabilitation. *Foot Ankle Int*. 2007 Feb;28(2):281-91.
- Easley ME, Adams SB Jr, Hembree WC, DeOrto JK. Results of total ankle arthroplasty. *J Bone Joint Surg Am*. 2011 Aug 3;93(15):1455-68.
- Undén A, Jheppsson L, Kamrad I, Carlsson Å, Henricson A, Karlsson MK, Rosengren BE. Better implant survival with modern ankle prosthetic designs: 1,226 total ankle prostheses followed for up to 20 years in the Swedish Ankle Registry. *Acta Orthop*. 2020 Apr;91(2):191-6.
- Zaidi R, Cro S, Gurusamy K, Siva N, Macgregor A, Henricson A, Goldberg A. The outcome of total ankle replacement: a systematic review and meta-analysis. *Bone Joint J*. 2013 Nov;95-B(11):1500-7.
- Labek G, Thaler M, Janda W, Agreiter M, Stöckl B. Revision rates after total joint replacement: cumulative results from worldwide joint register datasets. *J Bone Joint Surg Br*. 2011 Mar;93(3):293-7.
- Labek G, Todorov S, Iovanescu L, Stoica CI, Böhler N. Outcome after total ankle arthroplasty—results and findings from worldwide arthroplasty registers. *Int Orthop*. 2013 Sep;37(9):1677-82.
- Mercer J, Penner M, Wing K, Younger AS. Inconsistency in the Reporting of Adverse Events in Total Ankle Arthroplasty: A Systematic Review of the Literature. *Foot Ankle Int*. 2016 Feb;37(2):127-36.
- Spirit AA, Assal M, Hansen ST Jr. Complications and failure after total ankle arthroplasty. *J Bone Joint Surg Am*. 2004 Jun;86(6):1172-8.
- Wan DD, Choi WJ, Shim DW, Hwang Y, Park YJ, Lee JW. Short-term Clinical and Radiographic Results of the Salto Mobile Total Ankle Prosthesis. *Foot Ankle Int*. 2018 Feb;39(2):155-65.
- Cody EA, Scott DJ, Easley ME. Total Ankle Arthroplasty: A Critical Analysis Review. *JBJS Rev*. 2018 Aug;6(8):e8.
- Shane A, Sahli H. Total Ankle Replacement Options. *Clin Podiatr Med Surg*. 2019 Oct;36(4):597-607.
- Gaudot F, Colombier JA, Bonnin M, Judet T. A controlled, comparative study of a fixed-bearing versus mobile-bearing ankle arthroplasty. *Foot Ankle Int*. 2014 Feb;35(2):131-40.
- Nunley JA, Adams SB, Easley ME, DeOrto JK. Prospective Randomized Trial Comparing Mobile-Bearing and Fixed-Bearing Total Ankle Replacement. *Foot Ankle Int*. 2019 Nov;40(11):1239-48.
- Syed F, Ugwuoke A. Ankle arthroplasty: A review and summary of results from joint registries and recent studies. *EFORT Open Rev*. 2018 Jun 28;3(6):391-7.
- Valderrabano V, Pagenstert GI, Müller AM, Paul J, Henninger HB, Barg A. Mobile- and fixed-bearing total ankle prostheses: is there really a difference? *Foot Ankle Clin*. 2012 Dec;17(4):565-85.

17. New Zealand Joint Registry, New Zealand Orthopaedic Association. 2019. Accessed 07.11.19. <https://nzoa.org.nz/nzoa-joint-registry>.
18. Australian Orthopaedic Association National Joint Replacement Registry (AOANJRR). Demographics and Outcome of Ankle Arthroplasty: Supplementary Report. 2019.
19. Roukis TS, Elliott AD. Incidence of revision after primary implantation of the Salto® mobile version and Salto Talaris™ total ankle prostheses: a systematic review. *J Foot Ankle Surg*. 2015 May-Jun;54(3):311-9.
20. Conti SF, Wong YS. Complications of total ankle replacement. *Clin Orthop Relat Res*. 2001 Oct;(391):105-14.
21. Currier BH, Hecht PJ, Nunley JA 2nd, Mayor MB, Currier JH, Van Citters DW. Analysis of Failed Ankle Arthroplasty Components. *Foot Ankle Int*. 2019 Feb;40(2):131-8.
22. Terrier A, Fernandes CS, Guillemin M, Crevoisier X. Fixed and mobile-bearing total ankle prostheses: Effect on tibial bone strain. *Clin Biomech (Bristol, Avon)*. 2017 Oct;48:57-62.
23. Gross CE, Palanca AA, DeOrto JK. Design Rationale for Total Ankle Arthroplasty Systems: An Update. *J Am Acad Orthop Surg*. 2018 May 15;26(10):353-9.
24. Lefrancois T, Younger A, Wing K, Penner MJ, Dryden P, Wong H, Daniels T, Glazebrook M. A Prospective Study of Four Total Ankle Arthroplasty Implants by Non-Designer Investigators. *J Bone Joint Surg Am*. 2017 Feb 15;99(4):342-8.
25. Veljkovic AN, Daniels TR, Glazebrook MA, Dryden PJ, Penner MJ, Wing KJ, Younger ASE. Outcomes of Total Ankle Replacement, Arthroscopic Ankle Arthrodesis, and Open Ankle Arthrodesis for Isolated Non-Deformed End-Stage Ankle Arthritis. *J Bone Joint Surg Am*. 2019 Sep 4;101(17):1523-9.
26. Younger AS, Glazebrook M, Veljkovic A, Goplen G, Daniels TR, Penner M, Wing KJ, Dryden PJ, Wong H, Lalonde KA. A Coding System for Reoperations Following Total Ankle Replacement and Ankle Arthrodesis. *Foot Ankle Int*. 2016 Nov;37(11):1157-64.
27. Glazebrook MA, Arsenaault K, Dunbar M. Evidence-based classification of complications in total ankle arthroplasty. *Foot Ankle Int*. 2009 Oct;30(10):945-9.
28. de Keijzer DR, Joling BSH, Sierveit IN, Hoornenborg D, Kerkhoffs GMMJ, Haverkamp D. Influence of Preoperative Tibiotalar Alignment in the Coronal Plane on the Survival of Total Ankle Replacement: A Systematic Review. *Foot Ankle Int*. 2020 Feb;41(2):160-9.
29. Jensen J, Frøkjær J, Gerke O, Ludvigsen L, Torfing T. Evaluation of periprosthetic bone cysts in patients with a Scandinavian total ankle replacement: weight-bearing conventional digital radiographs versus weight-bearing multiplanar reconstructed fluoroscopic imaging. *AJR Am J Roentgenol*. 2014 Oct;203(4):863-8.
30. Besse JL. Osteolytic cysts with total ankle replacement: Frequency and causes? *Foot Ankle Surg*. 2015 Jun;21(2):75-6.
31. Dalat F, Barnoud R, Fessy MH, Besse JL; French Association of Foot Surgery AFCP. Histologic study of periprosthetic osteolytic lesions after AES total ankle replacement. A 22 case series. *Orthop Traumatol Surg Res*. 2013 Oct;99(6)(Suppl):S285-95.
32. Waizy H, Behrens BA, Radtke K, Almohallami A, Stukenborg-Colsman C, Bougoucha A. Bone cyst formation after ankle arthroplasty may be caused by stress shielding. A numerical simulation of the strain adaptive bone remodelling. *Foot (Edinb)*. 2017 Dec;33:14-9.
33. Espinosa N, Klammer G, Wirth SH. Osteolysis in Total Ankle Replacement: How Does It Work? *Foot Ankle Clin*. 2017 Jun;22(2):267-75.
34. Mehdi N, Bernasconi A, Laborde J, Lintz F. Comparison of 25 ankle arthrodeses and 25 replacements at 67 months' follow-up. *Orthop Traumatol Surg Res*. 2019 Feb;105(1):139-44.
35. Koo K, Liddle AD, Pastides PS, Rosenfeld PF. The Salto total ankle arthroplasty - Clinical and radiological outcomes at five years. *Foot Ankle Surg*. 2019 Aug;25(4):523-8.
36. Rodrigues-Pinto R, Muras J, Martín Oliva X, Amado P. Functional results and complication analysis after total ankle replacement: early to medium-term results from a Portuguese and Spanish prospective multicentric study. *Foot Ankle Surg*. 2013 Dec;19(4):222-8.
37. Schenk K, Lieske S, John M, Franke K, Mouly S, Lizée E, Neumann W. Prospective study of a cementless, mobile-bearing, third generation total ankle prosthesis. *Foot Ankle Int*. 2011 Aug;32(8):755-63.
38. Reuver JM, Dayerizadeh N, Burger B, Elmans L, Hoelen M, Tulp N. Total ankle replacement outcome in low volume centers: short-term followup. *Foot Ankle Int*. 2010 Dec;31(12):1064-8.
39. Bonnin M, Gaudot F, Laurent JR, Ellis S, Colombier JA, Judet T. The Salto total ankle arthroplasty: survivorship and analysis of failures at 7 to 11 years. *Clin Orthop Relat Res*. 2011 Jan;469(1):225-36.
40. Bonnin M, Judet T, Colombier JA, Buscayret F, Graveleau N, Piriou P. Midterm results of the salto total ankle prosthesis. *Clin Orthop Relat Res*. 2004 Jul;(424):6-18.
41. Marks RM. Mid-Term Prospective Clinical and Radiographic Outcomes of a Modern Fixed-Bearing Total Ankle Arthroplasty. *J Foot Ankle Surg*. 2019 Nov;58(6):1163-70.
42. Cody EA, Bejarano-Pineda L, Lachman JR, Taylor MA, Gausden EB, DeOrto JK, Easley ME, Nunley JA 2nd. Risk factors for failure of total ankle arthroplasty with a minimum five years of follow-up. *Foot Ankle Int*. 2019 Mar;40(3):249-58.
43. Pangrazzi GJ, Baker EA, Shaheen PJ, Okeagu CN, Fortin PT. Single-Surgeon Experience and Complications of a Fixed-Bearing Total Ankle Arthroplasty. *Foot Ankle Int*. 2018 Jan;39(1):46-58.
44. Stewart MG, Green CL, Adams SB Jr, DeOrto JK, Easley ME, Nunley JA 2nd. Midterm Results of the Salto Talaris Total Ankle Arthroplasty. *Foot Ankle Int*. 2017 Nov;38(11):1215-21.
45. Hofmann KJ, Shabin ZM, Ferkel E, Jockel J, Slovenkai MP. Salto Talaris Total Ankle Arthroplasty: Clinical Results at a Mean of 5.2 Years in 78 Patients Treated by a Single Surgeon. *J Bone Joint Surg Am*. 2016 Dec 21;98(24):2036-46.
46. Oliver SM, Coetzee JC, Nilsson LJ, Samuelson KM, Stone RM, Fritz JE, Giveans MR. Early patient satisfaction results on a modern generation fixed-bearing total ankle arthroplasty. *Foot Ankle Int*. 2016 Sep;37(9):938-43.
47. Chao J, Choi JH, Grear BJ, Tenenbaum S, Bariteau JT, Brodsky JW. Early radiographic and clinical results of Salto total ankle arthroplasty as a fixed-bearing device. *Foot Ankle Surg*. 2015 Jun;21(2):91-6.
48. Nodzo SR, Miladore MP, Kaplan NB, Ritter CA. Short to midterm clinical and radiographic outcomes of the Salto total ankle prosthesis. *Foot Ankle Int*. 2014 Jan;35(1):22-9.
49. Schweitzer KM, Adams SB, Viens NA, Queen RM, Easley ME, Deorio JK, Nunley JA. Early prospective clinical results of a modern fixed-bearing total ankle arthroplasty. *J Bone Joint Surg Am*. 2013 Jun 5;95(11):1002-11.
50. Gramlich Y, Neun O, Klug A, Buckup J, Stein T, Neumann A, Fischer S, Abt HP, Hoffmann R. Total ankle replacement leads to high revision rates in post-traumatic end-stage arthrosis. *Int Orthop*. 2018 Oct;42(10):2375-81.